

Sample Received: April 15, 2026

COA Issued: May 8, 2026

PRODUCT INFORMATION

Vendor:
DRYP TIDESSample Name:
ThermoxSample Type:
CapsuleLot Number:
THERMAP1-2026MW (g/mol):
290.3, 340.3

ANALYTICAL METHODS

Identity: Confirmed via MALDI-MS



Purity: RP-HPLC (214 nm)

Content: HPLC quantitation

TEST RESULTS

Specification	Result	Method	Status
Identity: Thermox (BAM-15, SLU-PP-332, CTS)	BAM-15, SLU-PP-332	MALDI-MS	✓ Conforms
Content		HPLC Quantitation	✓ Conforms
Overall Purity	99.7%	RP-HPLC (214 nm)	✓ Conforms
Endotoxin	< 0.05 EU/mL	<USP85>	✓ Conforms
Heavy Metals	< 0.001 ppm	< USP 232>	✓ Conforms

HPLC Chromatogram (Retention Time: 9.525, 11.500 min)

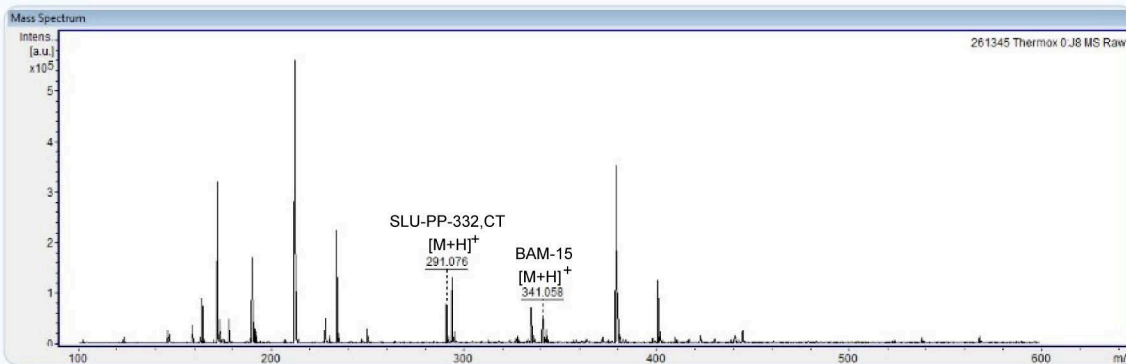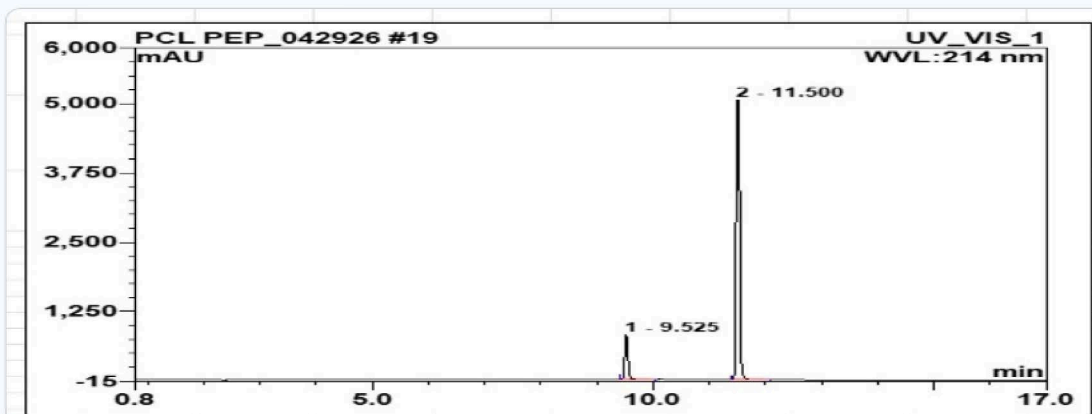

Certification: This COA confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Visit: <https://bioviridians.com/coa-search.html>*Shane Straight*Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.